


TEST REPORT
07-2017-BAL-212Met

Sample No. : Met-451
Type of Job : ON-SITE CALIBRATION
Date Calibrated : July 17, 2017
Sample : Dial-O-Gram Balance
Manufacturer : Ohaus
Serial No. : 0019/ AH9093
Graduation : 0.1 g
Capacity : 2 kg
Classification of Balance : Class II (High Accuracy Class)
Company : **SURIGAO STATE COLLEGE OF TECHNOLOGY**
Address : Narciso Street, Surigao City
Page : 1 of 3


This instrument was calibrated using reference standard traceable to SI Units as maintained by the National Metrology Institute- ITDI, Philippines. The following results were obtained:

I. Shift Test at 500 g

Position	Difference (g)	Maximum Permissible Error (MPE)
(1-2)	0.0	± 0.1 g
(1-3)	0.0	± 0.1 g
(1-4)	0.0	± 0.1 g
(1-5)	0.0	± 0.1 g

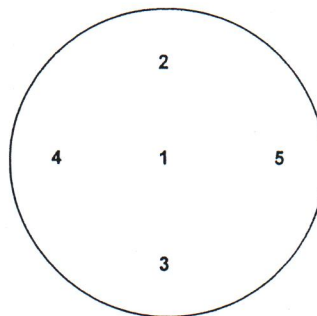

OP-026-F14
Revision 1



II. Repeatability Test at Half and Full Load


Load (g)	Difference (g)	Maximum Permissible Error (MPE)
500	0.0	± 0.1 g
1000	0.0	± 0.2 g

III. Departure from Nominal Value (Increasing & Decreasing Load)

Load (g)	Increasing Load Reading (g)	Error (g)	Decreasing Load Reading (g)	Error (g)	Maximum Permissible Error (MPE)	Uncertainty of Measurement (\pm g)
10	10.0	0.0	10.0	0.0	± 0.1 g	0.06
20	20.0	0.0	20.0	0.0	± 0.1 g	0.06
50	50.0	0.0	50.0	0.0	± 0.1 g	0.06
100	100.0	0.0	100.0	0.0	± 0.1 g	0.06
200	200.0	0.0	200.0	0.0	± 0.1 g	0.06
500	500.0	0.0	500.0	0.0	± 0.1 g	0.06
750	750.0	0.0	750.0	0.0	± 0.2 g	0.06
1000	1000.0	0.0	1000.0	0.0	± 0.2 g	0.06

Environmental Conditions : Relative Humidity : 49.0%
 Ambient Temperature : 25.6°C


Counter Weights	Number of Holes	Number of Leaded Holes
10 g	-	-
20 g (1)	-	-
20 g (2)	-	-
50 g	-	-
100 g	-	-
200 g (1)	-	-
200 g (2)	-	-
500 g	-	-




IV. Remarks:

1. The uncertainty of measurement is estimated at 95% level of confidence with a coverage factor $k=2$.
2. The above values are those obtained at the time of test and refer only to the particular instrument calibrated.
3. The end-user shall determine the suitability of this instrument for its intended use.
4. This report shall not be reproduced in any form, except in full, without written approval of the laboratory.


Calibrated by:


ENGR. MANOLITO R. TAPANGAN
Laboratory Analyst

Reviewed by:


GIDEON M. TANGHAL
Laboratory Analyst

Certified Correct and
Approved for Release by:


JENNIFER J. DEJARME
Chief Laboratory Analyst




TEST REPORT
07-2017-BAL-212Met

Sample No. : Met-452
Type of Job : ON-SITE CALIBRATION
Date Calibrated : July 17, 2017
Sample : Table Balance
Manufacturer : China
Serial No. : 0717B
Model : JPT-10
Graduation : 1 g
Capacity : 1000 g
Classification of Balance : Class III (Ordinary Accuracy Class)
Company : **SURIGAO STATE COLLEGE OF TECHNOLOGY**
Address : Narciso Street, Surigao City
Page : 1 of 3


This instrument was calibrated using reference standard traceable to SI Units as maintained by the National Metrology Institute- ITDI, Philippines. The following results were obtained:

I. Shift Test at 500 g

Position	Difference (g)	Maximum Permissible Error (MPE)
(1-2)	0.0	± 3.0 g
(1-3)	0.0	± 3.0 g
(1-4)	0.0	± 3.0 g
(1-5)	0.0	± 3.0 g

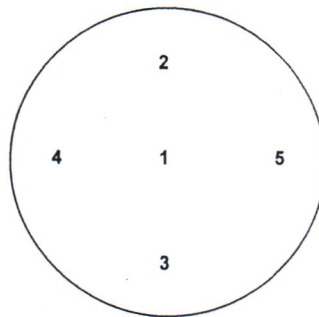

OP-026-F14
Revision 1



II. Repeatability Test at Half and Full Load


Load (g)	Difference (g)	Maximum Permissible Error (MPE)
500	0.0	± 3.0 g
1000	0.0	± 3.0 g

III. Departure from Nominal Value (Increasing & Decreasing Load)

Load (g)	Increasing Load Reading (g)	Error (g)	Decreasing Load Reading (g)	Error (g)	Maximum Permissible Error (MPE)	Uncertainty of Measurement (\pm g)
10	10.0	0.0	10.0	0.0	± 1.0 g	0.38
20	20.0	0.0	20.0	0.0	± 1.0 g	0.38
50	50.0	0.0	50.0	0.0	± 1.0 g	0.38
100	100.0	0.0	100.0	0.0	± 2.0 g	0.38
200	200.0	0.0	200.0	0.0	± 2.0 g	0.38
500	500.0	0.0	500.0	0.0	± 3.0 g	0.38
750	751.0	1.0	751.0	1.0	± 3.0 g	0.38
1000	1001.0	1.0	1001.0	1.0	± 3.0 g	0.38

Environmental Conditions : Relative Humidity : 56.0%
Ambient Temperature : 25.1°C


Counter Weights	Number of Holes	Number of Leaded Holes
10 g	-	-
20 g (1)	-	-
20 g (2)	-	-
50 g	-	-
100 g	-	-
200 g (1)	-	-
200 g (2)	-	-
500 g	-	-




IV. Remarks:

1. The uncertainty of measurement is estimated at 95% level of confidence with a coverage factor $k=2$.
2. The above values are those obtained at the time of test and refer only to the particular instrument calibrated.
3. The end-user shall determine the suitability of this instrument for its intended use.
4. This report shall not be reproduced in any form, except in full, without written approval of the laboratory.


Calibrated by:


ENGR. MANOLITO R. TAPANGAN
Laboratory Analyst

Reviewed by:


GIDEON M. TANGHAL
Laboratory Analyst

Certified Correct and
Approved for Release by:


JENNIFER J. DEJARME
Chief Laboratory Analyst




TEST REPORT
07-2017-BAL-212Met

Sample No. : Met-453
Type of Job : ON-SITE CALIBRATION
Date Calibrated : July 17, 2017
Sample : Dial-O-Gram Balance
Manufacturer : Ohaus
Serial No. : AH9081
Graduation : 0.1 g
Capacity : 2 kg
Classification of Balance : Class II (High Accuracy Class)
Company : **SURIGAO STATE COLLEGE OF TECHNOLOGY**
Address : Narciso Street, Surigao City
Page : 1 of 3


This instrument was calibrated using reference standard traceable to SI Units as maintained by the National Metrology Institute- ITDI, Philippines. The following results were obtained:

I. Shift Test at 500 g

Position	Difference (g)	Maximum Permissible Error (MPE)
(1-2)	0.0	± 0.1 g
(1-3)	0.0	± 0.1 g
(1-4)	0.0	± 0.1 g
(1-5)	0.0	± 0.1 g

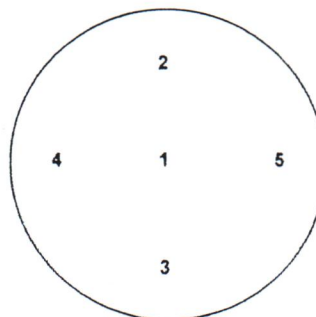

OP-026-F14
Revision 1



II. Repeatability Test at Half and Full Load


Load (g)	Difference (g)	Maximum Permissible Error (MPE)
500	0.0	± 0.1 g
1000	0.0	± 0.2 g

III. Departure from Nominal Value (Increasing & Decreasing Load)

Load (g)	Increasing Load Reading (g)	Error (g)	Decreasing Load Reading (g)	Error (g)	Maximum Permissible Error (MPE)	Uncertainty of Measurement (\pm g)
10	10.0	0.0	10.0	0.0	± 0.1 g	0.06
20	20.0	0.0	20.0	0.0	± 0.1 g	0.06
50	50.0	0.0	50.0	0.0	± 0.1 g	0.06
100	100.0	0.0	100.0	0.0	± 0.1 g	0.06
200	200.0	0.0	200.0	0.0	± 0.1 g	0.06
500	500.0	0.0	500.0	0.0	± 0.1 g	0.06
750	750.0	0.0	750.0	0.0	± 0.2 g	0.06
1000	1000.0	0.0	1000.0	0.0	± 0.2 g	0.06

Environmental Conditions : Relative Humidity : 49.0%
Ambient Temperature : 25.5°C


Counter Weights	Number of Holes	Number of Leaded Holes
10 g	-	-
20 g (1)	-	-
20 g (2)	-	-
50 g	-	-
100 g	-	-
200 g (1)	-	-
200 g (2)	-	-
500 g	-	-




IV. Remarks:

1. The uncertainty of measurement is estimated at 95% level of confidence with a coverage factor $k=2$.
2. The above values are those obtained at the time of test and refer only to the particular instrument calibrated.
3. The end-user shall determine the suitability of this instrument for its intended use.
4. This report shall not be reproduced in any form, except in full, without written approval of the laboratory.

Calibrated by:



ENGR. MANOLITO R. TAPANGAN
Laboratory Analyst

Reviewed by:


GIDEON M. TANGHAL
Laboratory Analyst

Certified Correct and
Approved for Release by:


JENNIFER J. DEJARME
Chief Laboratory Analyst




TEST REPORT
07-2017-BAL-212Met

Sample No. : Met-454
Type of Job : ON-SITE CALIBRATION
Date Calibrated : July 17, 2017
Sample : Table Balance
Manufacturer : China
Serial No. : 0009
Graduation : 1 g
Capacity : 1000 g
Classification of Balance : Class III (Ordinary Accuracy Class)
Company : **SURIGAO STATE COLLEGE OF TECHNOLOGY**
Address : Narciso Street, Surigao City
Page : 1 of 3

This instrument was calibrated using reference standard traceable to SI Units as maintained by the National Metrology Institute- ITDI, Philippines. The following results were obtained:

I. Shift Test at 500 g

Position	Difference (g)	Maximum Permissible Error (MPE)
(1-2)	0.0	± 3.0 g
(1-3)	0.0	± 3.0 g
(1-4)	0.0	± 3.0 g
(1-5)	0.0	± 3.0 g

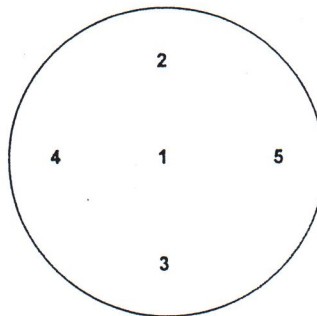

OP-026-F14
Revision 1